

Instructions for Use


1 mL Sperm Purification Device

Device Components:

- VetCount™ Harvester 1 mL Sperm Purification Device
- Instructions for Use
- Accessories: 3 x 1 mL Syringes

Equipment required, but not supplied:

- Sperm Preparation Medium
- 37°C or 98.6°F incubator

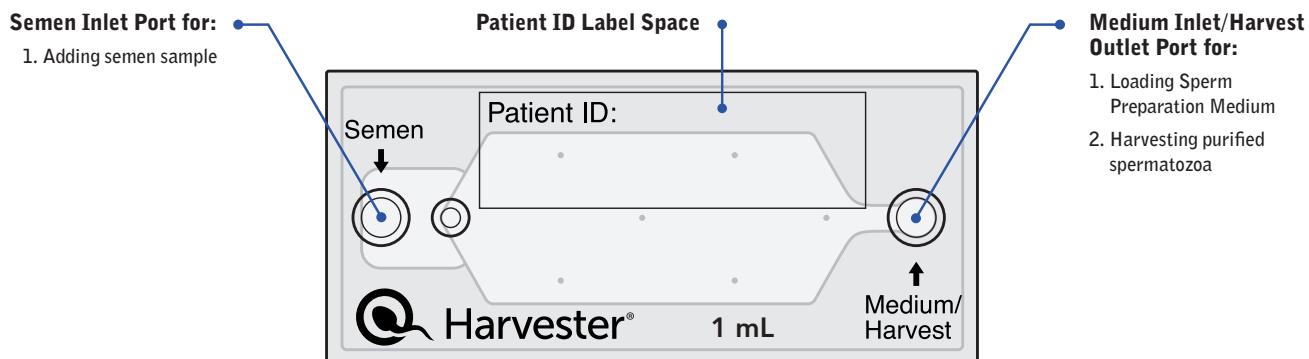

Important Information

Please read detailed Instructions before use:

- Carefully adhere to the recommended volumes for each step
- Avoid both over- and/or underfilling of the device
- If spillage of sample occurs (resulting in less than a 1 mL sample) empty out the remaining sample in the collection, and start over filling the syringe with sample.
- Always load and aspirate the VetCount™ Harvester device placed on a horizontal surface
- When moving the device to/from the incubator then keep the device on a horizontal surface
- The device is for single-use, only
- The VetCount™ Harvester comes sterile and a possible contamination from for example the work environment might decrease the efficiency of the VetCount™ Harvester
- Practice universal precautions when handling human body fluids such as semen. Follow the guide lines described in the WHO laboratory manual for the examination and processing of human semen
- The device should be used only by properly trained operators
- Re-use of the device may lead to:
 - less efficient purification of the sample
 - contamination (e.g. two different semen samples)


2 Aspirating the semen sample

Before aspirating the semen sample, it must be homogeneous.

Aspirate 1 mL of the semen sample using one of the included syringes. Avoid any air bubbles.

If there is insufficient semen sample volume then add Sperm Preparation Medium* to bring the volume to 1 mL.

NOTE: If using a frozen semen sample then follow the instructions from the Sperm Bank for thawing.

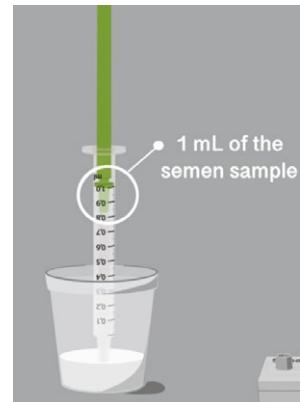


* Preparation of the Medium as informed by the manufacturers of the sperm preparation medium

3 Inject the sample into the device

Place the 1 mL syringe filled with the semen sample into the Semen Inlet port.

Press the plunger of the syringe slowly and release the semen sample into the device.


NOTE: Always handle the device on a flat horizontal surface (table).

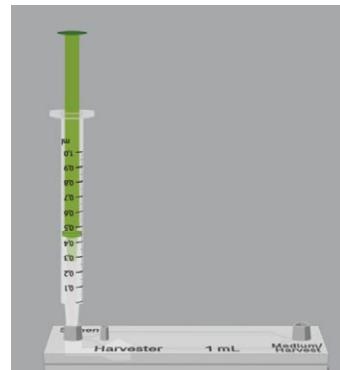

1 Preparing the semen sample

Make sure that the semen sample is liquefied.


Gather all the equipment needed and work on a clean surface.



4 Add the Sperm Preparation Medium

Use another 1 mL syringe and aspirate 0.8 mL Sperm Preparation Medium. Avoid any air bubbles.


Place the syringe in the Medium Inlet Port and release slowly the Sperm Preparation Medium.

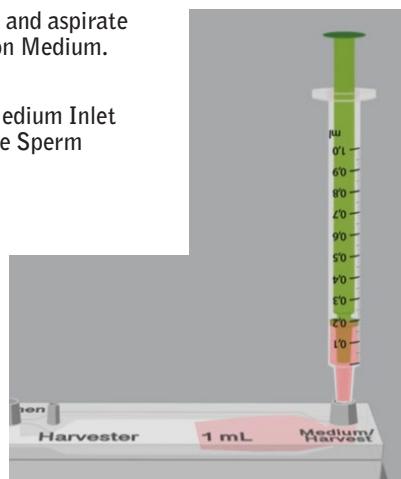

6 Harvest

Remove the device from the Incubator.

Use another 1 mL syringe and place it in the Harvest Outlet Port and aspirate 0.8 mL of the purified semen sample.*

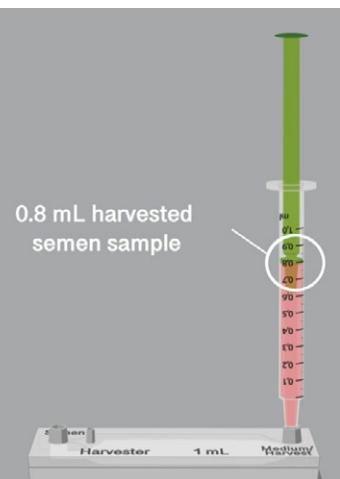


*NOTE: Appr. 90-95% of the purified semen sample can be aspirated. Do not tilt the device in order to get the remaining 5-10% out.

5 Incubation


Incubate the device for 30 Min at 37°C or 98.6°F.

Keep the device horizontally at all times.

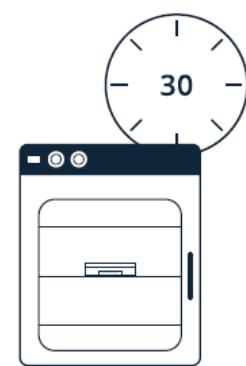

7 The harvested sample is ready to be used

The harvested Progressive Motile Sperm Cells (PMSCs) are ready to be used.

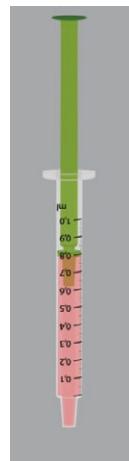

Device Description:

The VetCount™ Harvester is a Sperm Purification Device. The device purifies the sperm sample by allowing only Progressive Motile Sperm Cells (PMSCs) to pass the device's membrane system. The VetCount™ Harvester has a design/technology that utilizes the progressive motility of the sperm cells to separate the PMSCs from the rest of the sperm population.

The device consists of 3 components:

- Sample compartment 1 mL
- Medium/Swim-Up compartment 0.8 mL
- Micropore filter 10 µm

The device is used for Animal Assisted Reproductive Technology (ART).

Intended Purpose:

The intended purpose of the VetCount™ Harvester is to purify semen samples and select for Progressive Motile Sperm Cells (PMSCs), and thereby be used in support of conception as part of Animal Assisted Reproductive Technology (ART).

Sterilization:

The sterilization method used for the device is gamma radiation, at a dose level of 25kGy to 39kGy.

The device is radiation-sterilized with a sterility assurance level (SAL) of 10⁻⁶. It is individually packaged and for single-use only.

Storage:

Store at 6°C - 37°C / 42.8°F - 98.6°F.

Disposal:

Discard the used device and materials as medical waste.

Manufactured by:

MotilityCount ApS
Gl. Køge Landevej 57, 2.
DK-2500 Valby
Denmark
www.motilitycount.com

REF INT1011.4

Date of Issue: 2024-06-12

Contact:

If you have any questions, please contact us at: info@vetcount.com

In case any serious incident has occurred in relation to the device, it shall be reported to the manufacturer and the competent authority of the Member State.

 Manufacturer

 Expiration Date yyyy.mm.dd

 Lot Number

 Catalogue Number

 **STERILE** **R** Sterilized Using Irradiation

 Do Not Resterilize

 Do Not Use if Package is Damaged

 Medical Device

 Fragile Item, Handle Carefully

 Keep away from direct sunlight

 Keep Dry

 37°C
98.6°F
6°C
42.8°F
Storage Temperature Limits

 Do Not Reuse

 Consult Instruction For Use

Patents and Trademarks:

VetCount™ and the Sperm Cell symbol are trademarks of MotilityCount ApS.

Patent: PCT WO2014/177157